

A Highly Sensitive Luminescent Biosensor for the Microvolumetric Detection of the *Pseudomonas aeruginosa* Siderophore Pyochelin

Daniela Visaggio,^{*,‡} Mattia Pirolo,[‡] Emanuela Frangipani, Massimiliano Lucidi, Raffaella Sorrentino, Emma Mitidieri, Francesca Ungaro, Andrea Luraghi, Francesco Peri, and Paolo Visca^{*}



Cite This: *ACS Sens.* 2021, 6, 3273–3283



Read Online

ACCESS |



Metrics & More




Article Recommendations



Supporting Information

ABSTRACT: The pyochelin (PCH) siderophore produced by the pathogenic bacterium *Pseudomonas aeruginosa* is an important virulence factor, acting as a growth promoter during infection. While strong evidence exists for PCH production *in vivo*, PCH quantification in biological samples is problematic due to analytical complexity, requiring extraction from large volumes and time-consuming purification steps. Here, the construction of a bioluminescent whole cell-based biosensor, which allows rapid, sensitive, and single-step PCH quantification in biological samples, is reported. The biosensor was engineered by fusing the promoter of the PCH biosynthetic gene *pchE* to the *luxCDABE* operon, and the resulting construct was inserted into the chromosome of the $\Delta pvdA\Delta pchD\Delta fpvA$ siderophore-null *P. aeruginosa* mutant. A bioassay was setup in a 96-well microplate format, enabling the contemporary screening of several samples in a few hours. A linear response was observed for up to 40 nM PCH, with a lower detection limit of 1.64 ± 0.26 nM PCH. Different parameters were considered to calibrate the biosensor, and a detailed step-by-step operation protocol, including troubleshooting specific problems that can arise during sample preparation, was established to achieve rapid, sensitive, and specific PCH quantification in both *P. aeruginosa* culture supernatants and biological samples. The biosensor was implemented as a screening tool to detect PCH-producing *P. aeruginosa* strains on a solid medium.

KEYWORDS: bioluminescence, biosensor, luciferase, pyochelin, *Pseudomonas aeruginosa*, siderophore



Tissues and biological fluids of mammals are protected from invading pathogens by iron-binding proteins, which represent major components of the innate immunity.¹ Therefore, during infection, bacteria are faced with a tremendous iron-starvation stress, which is inductive of siderophore (iron chelator) synthesis.^{2–4} The Gram-negative bacterium *Pseudomonas aeruginosa* is one of the most dreaded opportunistic pathogens in the hospital setting and represents the first cause of morbidity and mortality in cystic fibrosis (CF) patients.⁵ *P. aeruginosa* produces two siderophores, namely, pyoverdine (PVD) and pyochelin (PCH), which are endowed with very different structural and functional properties and capable of chelating Fe(III) with different affinities.^{6,7}

PVD is a dihydroxyquinoline-containing green fluorescent peptide showing very high affinity for Fe(III) ($K_f = 10^{32} \text{ M}^{-1}$).^{8,9} The role of PVD in *P. aeruginosa* pathogenicity has extensively been studied, since PVD is produced in large amounts and can easily be quantified both *in vitro* and *in vivo*, thanks to its strong fluorescence emission.^{10,11}

PCH is the second siderophore produced by *P. aeruginosa*¹² and originates from the enzymatic condensation of salicylic acid with two cysteine molecules.^{13,14} The PCH structure


contains three asymmetric carbons (C-4', C-2'', C-4'') and exists as a mixture of the two interconvertible diastereomers PCH I (4'R, 2''R, 4''R) and PCH II (4'R, 2''S, 4''R).¹⁵ Its affinity for Fe(III) is 10^{28} M^{-2} .¹⁶

The PCH biosynthetic genes are organized in two operons, *pchDCBA* and *pchEFGHI*.¹⁷ A third operon, *fptABCX*, encodes the FptA outer membrane receptor and the FptX inner membrane permease, which mediate active transport of PCH inside the *P. aeruginosa* cell.¹⁸ In the cytoplasm, the PCH-Fe(III) complex binds the PchR regulator, which induces the expression of the PCH biosynthesis and uptake operons.¹⁹ PchR is a protein belonging to the AraC/XylS family of transcriptional regulators, which act as repressors or activators of gene expression depending on the absence or presence of a specific effector molecule, respectively. In particular, genes

Received: May 17, 2021

Accepted: August 11, 2021

Published: September 3, 2021



implicated in PCH biosynthesis and uptake are repressed by PchR in the absence of cytoplasmic PCH, while they are induced when PchR is activated upon PCH-(FeIII) binding.^{20,21} Since an excess of cytoplasmic iron is toxic for bacterial cells, all *P. aeruginosa* iron acquisition systems are repressed under iron-replete conditions by the binding of the ferric uptake regulator protein (Fur) to the promoter regions of PVD and PCH biosynthesis and uptake genes.^{14,22} This highly specific regulatory circuitry ensures PCH production when (i) cells are iron starved (hence, Fur repression is relieved) and (ii) PCH is effective in feeding the cell with iron (hence, PchR binds cytoplasmic PCH-Fe(III), activates PCH biosynthesis, and transport genes).

PCH has a major impact on *P. aeruginosa* pathogenesis, as it contributes to overcoming the iron starvation response of the host during bacterial infection.²³ PCH is crucial for feeding *P. aeruginosa* cells with iron and contributes to pathogenicity in a mouse model of lung infection.²⁴ Indirect evidence of *in vivo* expression of PCH biosynthesis genes was inferred from transcriptional profiling of *P. aeruginosa* during septicemia, urinary tract, lung, and wound infections,^{25–28} and the PCH transport gene *fptA* was identified among the most highly expressed virulence genes *in vivo*.²⁹ However, *in vivo* detection of PCH is problematic, and PCH production during *P. aeruginosa* infection was occasionally documented in CF sputum samples, which showed significant induction of *pch* genes.^{11,26} *In vitro* studies suggest that PCH is also responsible for secondary pathogenic effects on host tissues through the generation of hydroxyl radicals in combination with pyocyanin, which is an extracellular phenazine compound produced by *P. aeruginosa*.^{30,31}

The paucity of information about PCH production levels during *P. aeruginosa* infection is due to the complexity of available methods to quantify this siderophore in biological samples. At present, PCH quantification methods rely on solvent extraction followed by concentration of the extract and PCH purification and detection by thin-layer chromatography, spectrofluorimetry, or HPLC.^{14,32–34} These methods are time-consuming, require handling of hazardous solvents and specialized equipment for PCH extraction and quantification, respectively, and unavoidably cause non-negligible loss of material, which could ultimately result in the underestimation of the PCH concentration.

In this study, we report the construction of a bioluminescent whole cell-based biosensor for the rapid, specific, and single-step quantification of PCH, overcoming the numerous drawbacks of current PCH detection methods. The sensitivity, range of linear response, and specificity of the biosensor were experimentally determined. The biosensor was developed in the 96-well microtiter plate format and successfully used for PCH quantification in *P. aeruginosa* culture supernatants and biological samples, then adapted to the agar plate format for the qualitative screening of PCH-producing *P. aeruginosa* clinical isolates.

EXPERIMENTAL SECTION

Bacterial Strains and Growth Media. Bacterial strains and plasmids used in this study are listed in Table S1. *Escherichia coli* and *P. aeruginosa* were grown in Luria-Bertani broth (LB)³⁵ and LB agar plates. The *P. aeruginosa* biosensor strain $\Delta pvdA\Delta pchD\Delta fvpA$ *PpchE::lux* is freely available to the scientific community and can be provided upon request to the corresponding authors. When required, antibiotics were used at the following concentrations: ampicillin (Ap,

100 $\mu\text{g}/\text{mL}$), tetracycline (Tc, 12.5 $\mu\text{g}/\text{mL}$), and gentamicin (Gm, 10 $\mu\text{g}/\text{mL}$) for *E. coli*; Gm (200 $\mu\text{g}/\text{mL}$), carbenicillin (Cb, 250 $\mu\text{g}/\text{mL}$), and Tc (100 $\mu\text{g}/\text{mL}$) for *P. aeruginosa*. *P. aeruginosa* strains were also grown in the iron-poor casamino acid (DCAA) medium³⁶ and in casamino acid (CAA) agarose plates (10 g/L CAA, Difco; 15 g/L Certified Molecular Biology Agarose, Bio-Rad).

PVD Extraction and Quantification. PVD produced by *P. aeruginosa* strains was quantified after 24 h growth at 37 °C in DCAA by measuring the absorbance at 405 nm of culture supernatants appropriately diluted in 0.1 M Tris-HCl, pH 8.0. Values were normalized to the cell density of the bacterial culture (OD_{600}), as previously described.³⁷ PVD was purified as previously described.³⁸ Briefly, *P. aeruginosa* $\Delta pchD$ was grown in DCAA for 24 h. The culture supernatant was purified by filtration through a Sep-Pak C18 Vac-Cartridge 3 cc (Waters). The filtered culture supernatant containing PVD was loaded and washed with double-distilled water to remove unwanted components. PVD was then eluted with 50% (vol/vol) methanol, evaporated to dryness in a desiccator, and dissolved in a small volume of double distilled water. The PVD concentration was determined by spectrophotometric measurement of the apo form at OD_{405} ($\epsilon = 1.4 \times 10^4 \text{ M}^{-1} \text{ cm}^{-1}$).

PCH Extraction and Quantification. PCH was extracted from *P. aeruginosa* $\Delta pvdA$ by the ethyl acetate extraction of acidified 36 h-old culture supernatants in DCAA. Briefly, the supernatant was adjusted to pH 1.5–2.0 with 1 N HCl and extracted with 1 volume of ethyl acetate.³⁹ After evaporation of the organic phase, the dry residue was suspended in 100 μL of methanol. PCH extracts were purified by an automatized reverse-phase chromatographer equipped with a UV-vis detector (BIOTAGE Isolera One Flash Chromatography System, RP-C18 column, gradient water/methanol). The amount of apo-PCH was determined by spectrophotometric measurement at OD_{330} ($\epsilon = 4400 \text{ M}^{-1} \text{ cm}^{-1}$).⁴⁰ A 40 mM of stock solution of PCH was prepared in dimethyl sulfoxide (DMSO) and stored at -20 °C until used. The ethyl acetate extract of PAO1, $\Delta pvdA$, $\Delta pchD$, and *P. aeruginosa* TR1 was also applied to a silica gel G (60F254) thin-layer chromatography (TLC) plate (Merck) using acetone:methanol:0.2 M acetic acid (5:2:1) as the mobile phase.⁴¹ PCH from TLC plates was qualitatively characterized by (i) yellow-green fluorescence emission under UV light⁴² and (ii) iron-binding capacity when sprayed with 0.1 M FeCl_3 in 0.1 M HCl resulting in red-brown spots.⁴²

Chemical Synthesis of PCH and Enantio-PCH. The two enantiomers *N*-methyl-L-cysteine and *N*-methyl-D-cysteine, which are required in the final step of PCH and enantio-PCH chemical synthesis, were prepared according to literature procedures,^{43,44} starting from commercially available L- or D-cysteine. In this synthetic procedure (Figure S1), cysteine enantiomers were separately reacted with trityl alcohol in TFA to protect the thiol group as S-trityl, and then the amine group was protected as *tert*-butoxycarbonyl (Boc) carbamate that, after *N*-methylation with methyl iodide, gave the fully protected S-trityl, *N*-Boc, *N*-methyl L- or D-cysteine. The simultaneous deprotection of amino and thiol groups (Boc and trityl cleavage, respectively) gave the final *N*-methyl-L- or D-cysteine. PCH and enantio-PCH were then synthesized using the literature protocol⁴⁵ over four steps (Figure S2). Commercially available 2-hydroxybenzoxynitrile was condensed with L-cysteine providing the thiazolidine intermediate. The treatment of the thiazolidine intermediate with *N*-methyl-*O*-methyl hydroxylamine in the presence of condensing agents afforded the corresponding Weinreb amide, and the subsequent reduction with lithium aluminum hydride (LAH) gave aldehyde as a racemic mixture. The final condensation of aldehyde with the previously synthesized *N*-methyl-L-cysteine or its enantiomer *N*-methyl-D-cysteine followed by spontaneous cyclization gave PCH and enantio-PCH, respectively, as a mixture of four diastereomers (Figure S2).

Generation of Plasmids and Reporter Strains. Unmarked in-frame deletion mutants in *fvpA* and *pchR* genes were constructed by suicide plasmid insertion mutagenesis. *E. coli* was used for recombinant DNA manipulations. The constructs for mutagenesis were generated by directional cloning into the pDM4 or pME3087 vector (Table S1)^{46,47} of two DNA fragments of ~ 600 bp,

encompassing the regions upstream and downstream of the sequence to be deleted. Fragments were amplified by PCR, digested with the appropriate restriction enzymes, and cloned into pDM4 or pME3087, generating the derivative vectors pDM4 Δ fvpA and pME3087 Δ pchR (Table S1). PCR primers and restriction enzymes used for cloning of PCR products are listed in Table S2. All constructs were verified by DNA sequencing. Deletion vectors were conjugally transferred from *E. coli* S17.1 λ pir into the *P. aeruginosa* suitable deletion mutants (Table S1). The in-frame deletion mutations were obtained by recombination, as previously described.^{46,47} All the deletion events were verified by PCR using primers flanking the deleted region and amplicon sequencing. For the generation of mini-CTX PpchE::lux insertion, a DNA fragment encompassing the pchE promoter was amplified using the primers listed in Table S2 from the *P. aeruginosa* PAO1 chromosome. The amplicon was digested with BamHI-HindIII and ligated in the mini-CTX-lux plasmid. The resulting mini-CTX PpchE::lux was transferred from *E. coli* S17.1 λ pir into *P. aeruginosa* strains by conjugation. Excision of the mini-CTX plasmid was achieved by Flp-mediated recombination via pFLP2, as previously described.⁴⁸

Biosensor Response to PCH and Other Iron-Binding Compounds. To test the biosensor response to PCH, *P. aeruginosa* PAO1 Δ pvdA Δ pchD Δ fvpA PpchE::lux was grown for 16 h at 37 °C in DCAA supplemented with 1 μ M FeCl₃. To exclude any iron carryover, the cells were washed with saline prior to being suspended in DCAA. The biosensor strain PAO1 Δ pvdA Δ pchD Δ fvpA PpchE::lux was inoculated at final OD₆₀₀ of 1, 0.5, and 0.25 into black, clear-bottom 96-wells microtiter plates (Greiner) in the presence of an increasing concentration of purified PCH. Different inoculum volumes (200, 100, and 50 μ L) were tested in the assay. OD₆₀₀ and light count per second (LCPS) were monitored every 15 min in a Tecan Spark 10 M multilabel plate reader (Tecan, Männedorf, Switzerland) for up to 6 h at 25 °C. Once the optimal biosensor assay condition is defined (OD₆₀₀ = 0.25; final volume 50 μ L per well), these parameters were applied in all subsequent assays. The limit of detection (LOD) and the limit of quantification (LOQ) of the PCH biosensor were determined according to the equations: LOD = 3 × (SD/S) and LOQ = 10 × (SD/S),^{49,50} where SD is the standard deviation of the blank value (n = 10 replicates) and S is the slope of the calibration curve (*i.e.*, the sensitivity). The biosensor response was also assessed in the presence of chemically synthesized PCH and enantio-PCH, purified PVD, sodium salicylate (Sigma), deferoxamine (Desferal; Novartis), deferiprone (3-hydroxy-1,2-dimethylpyridin-4(1H)-one; Sigma-Aldrich), and FeCl₃ (Sigma) at the indicated concentrations.

Biological Fluids and CF Sputa. Sputum and first-morning urine specimens were collected from 10 healthy donors who tested culture-negative for *P. aeruginosa*. Each fluid was pooled, centrifuged (13,000g, 10 min, 4 °C), and sterilized through a 0.20 μ m filter. Sterile artificial tears (Irilens 0.4%) were purchased from Montefarmaco (Italy). In addition, sputa from eight anonymous CF patients were provided by the clinical microbiology laboratory of Policlinico Umberto I, Rome (Italy), and processed as described above. Biological samples were stored at −20 °C until the assay.

PCH Quantification in *P. aeruginosa* Culture Supernatants and Biological Fluids. PCH detection in culture supernatants of *P. aeruginosa* strains and biological fluids (including CF sputa) was performed using the *P. aeruginosa* Δ pvdA Δ pchD Δ fvpA PpchE::lux biosensor. *P. aeruginosa* strains (listed in Table S1) were grown for 24 h at 37 °C in DCAA. The culture supernatants were collected, filtered through a Millipore membrane (pore size 0.45 μ m, Sarstedt), and stored at −20 °C until used. Five microliters of appropriate dilutions of culture supernatants or biological fluids were added to 45 μ L of DCAA inoculated with the biosensor strain (final OD₆₀₀ = 0.25). Microtiter plates were incubated at 25 °C, and OD₆₀₀ and LCPS were measured after 3.5 h using a Tecan Spark 10 M multilabel plate reader. A calibration curve was generated with purified PCH at known concentrations (5–320 nM) and used to calculate the concentration of PCH in each sample.

Detection of PCH and Siderophores on Agar Plates. Single colonies of different *P. aeruginosa* strains (listed in Table S1) were cultured for 8 h in LB at 37 °C. Bacteria were washed in saline, diluted to OD₆₀₀ = 0.1, and 5 μ L of each bacterial suspension was spotted onto casamino acid (CAA) agarose plate (5 g/L CAA and 15 g/L agarose). After 24 h incubation at 37 °C, PVD production was detected under UV light, and cells were killed through exposure to chloroform vapors for 15 min. Plates were then subsequently overlaid with CAA soft agarose (5 g/L casamino acids, Difco; 7.5 g/L agarose Bio-Rad) containing the biosensor strain (OD₆₀₀ = 0.5). After incubation at 37 °C for 1 h, plates were visualized with a ChemiDoc XRS+ Imaging System (Bio-Rad), using a 3 min exposure time.

RESULTS AND DISCUSSION

Design and Construction of a PCH-Responsive Whole Cell-Based Biosensor. To generate a biosensor capable of quantifying PCH at the nanomolar level, the luxCDABE operon, encoding the luciferase enzyme from the bacterium *Photobacterium luminescens*, was chosen as the reporter system, being characterized by a high signal/noise ratio and not requiring supplementation with an exogenous substrate for signal (blue photon) emission.^{51,52} A transcriptional fusion between the PchR-dependent PpchE promoter and the luxCDABE operon was generated and integrated in the attB neutral chromosomal site in the *P. aeruginosa* Δ pvdA Δ pchD Δ fvpA triple mutant⁵³ (Figure 1). This recipient




Figure 1. Schematic of the PCH-responsive whole cell-based biosensor. A transcriptional fusion between the pchE promoter (PpchE) and the luxCDABE operon was integrated in the chromosome of the *P. aeruginosa* Δ pvdA Δ pchD Δ fvpA mutant. Fe(III)-PCH is actively transported in the cytoplasm via FpTAX, where it binds the transcriptional regulator PchR and directs the expression of the PpchE::lux fusion, eliciting bioluminescence emission. The Fe(II)-bound ferric uptake regulator Fur and PCH-unloaded PchR repress the expression of the PpchE::lux fusion. T-shaped lines represent negative control of PpchE.

strain is a siderophore null mutant, *i.e.*, impaired in the synthesis of both PVD and PCH, and is also unable to uptake PVD due to the absence of the FpvA receptor. The inability to produce siderophores prevents PpchE auto-induction by endogenously synthesized PCH. Moreover, the lack of the PVD transporter FpvA prevents the entrance of exogenous PVD into the biosensor cell, thus avoiding the repression of the PpchE::lux fusion by Fe(III) delivered through the Fe(III)-PVD uptake pathway. However, the Δ pvdA Δ pchD Δ fvpA mutant still produces both FptA and FptX transporters, so it has no defect in PCH uptake from the extracellular milieu. Consequently, we predicted (i) the bioluminescence emission of the whole-cell biosensor to be dependent on the levels of exogenously added PCH, which is transported intracellularly

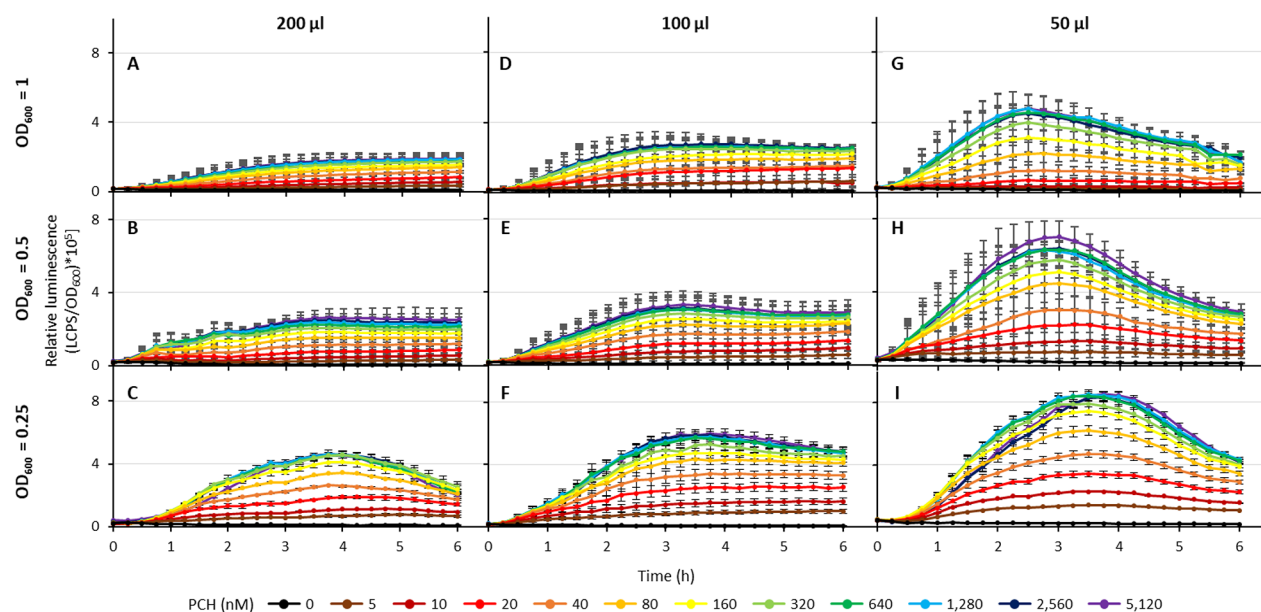


Figure 2. Effect of reporter cell density and assay volume on the biosensor response to PCH. Relative light emission (LCPS/ OD_{600}) by the *P. aeruginosa* $\Delta pvdA\Delta pchD\Delta fpvA$ mutant carrying the *PpchE::lux* fusion, in response to increasing PCH concentrations, ranging from 5 to 5120 nM. LCPS and OD_{600} were measured every 15 min for 6 h at 25 °C. Bacteria were inoculated at three different cell densities and three final volume combinations: (A) 200 μ L, $OD_{600} = 1$; (B) 200 μ L, $OD_{600} = 0.5$; (C) 200 μ L, $OD_{600} = 0.25$; (D) 100 μ L, $OD_{600} = 1$; (E) 100 μ L, $OD_{600} = 0.5$; (F) 100 μ L, $OD_{600} = 0.25$; (G) 50 μ L, $OD_{600} = 1$; (H) 50 μ L, $OD_{600} = 0.5$; (I) 50 μ L, $OD_{600} = 0.25$. Data are the mean of three independent experiments \pm SD.

and serves as inducer of the *PpchE::luxCDABE* promoter-probe gene fusion, and (ii) the bioluminescence emission to be proportional to the PCH concentration (Figure 1).

Experimental Setup for the Use of the Bioluminescent Whole Cell-Based Biosensor. The expression of *pch* (PCH biosynthesis) genes and, consequently, of the *PpchE::luxCDABE* reporter fusion is repressed by Fur under iron replete conditions. This is because the *PpchE* promoter contains a Fur-Fe(II)-binding region, which abrogates the transcriptional activity under conditions of iron availability.²²

In order to prevent Fur-Fe(II)-mediated repression of the biosensor, the iron-poor medium DCAA³⁶ was chosen for setting the operational conditions of the bioluminescent biosensor. Although iron scarcity is essential for studying the biosensor response to PCH, too severe iron limitation imposed by DCAA (<0.5 μ M)³⁶ would suppress the growth of a siderophore-null *P. aeruginosa* mutant. Therefore, the minimum non-limiting iron concentration allowing the $\Delta pvdA\Delta pchD\Delta fpvA$ mutant to grow similarly to the wild type, without causing complete repression of iron uptake genes, was initially investigated. To this purpose, the growth of the biosensor strain and wild-type PAO1 was monitored for 24 h in DCAA supplemented with increasing $FeCl_3$ concentrations (from 0.5 to 8 μ M), and PVD production by wild-type PAO1 was measured as an indicator of iron-repressible gene expression. *P. aeruginosa* PAO1 grew poorly in the absence of exogenously added iron, and the $\Delta pvdA\Delta pchD\Delta fpvA$ mutant grew even less (Figure S3A,B). However, the addition of 1 μ M $FeCl_3$ supported the sufficient growth of both strains without abrogating PVD production by wild-type PAO1 (Figure S3C). Therefore, biosensor cells were cultivated for 24 h in DCAA supplemented with 1 μ M $FeCl_3$, since this iron concentration does not shut off the expression of Fur-Fe(II)-repressible genes (*i.e.*, *pvd* and *pch* genes).

To set the optimal experimental conditions for luminescence detection, three cell densities ($OD_{600} = 1.0$; 0.5; 0.25) and three different volumes of the bacterial suspension (200, 100, and 50 μ L) were tested in a 96-well microtiter plate assay. All the experiments were performed in DCAA supplemented with purified PCH from *P. aeruginosa* PAO1 (concentration range 5 to 5120 nM), and the relative bioluminescence emission was monitored every 15 min for 6 h (Figure 2). To minimize the growth of the biosensor strain, the temperature was set at 25 °C during the assay. Interestingly, the lowest cell density ($OD_{600} \approx 0.25$) and the smallest volume (50 μ L) provided the highest relative light emission, expressed as light counts per second (LCPS)/ OD_{600} of the cell suspension (Figure 2I), indicating that the assay volume influences the amount of light detectable per cell and hence the biosensor response. This result can be explained by the multiple scattering effect that occurs when the concentration of particles (*i.e.*, cells) is too high. In this case, the measured OD_{600} does not linearly increase with the cell number, and the Beer–Lambert law is no longer a valid approximation. In addition, the bioluminescent photons are scattered by overlying cells and are deflected away from the photodetector.⁵⁴ This is because bacteria located in the upper layers shield the light signal emitted by the bacteria underneath. In fact, the higher the volume, the higher the optical path of the well, hence the light shielding by the bacterial suspension. Lowering the reaction volumes and cell densities enhanced the relative performance of the biosensor, expressed as LCPS/ OD_{600} . An optimal dose-dependent response of the biosensor was observed using the lowest cell density ($OD_{600} \approx 0.25$) and the smallest assay volume (50 μ L) within the 5–160 nM PCH concentration range. PCH concentrations of >160 nM caused a moderate increase in light emission (Figure 2I). This phenomenon is likely due to the fact that PCH concentrations higher than 160 nM saturate the FptA/FptX transporters and/or the transcriptional

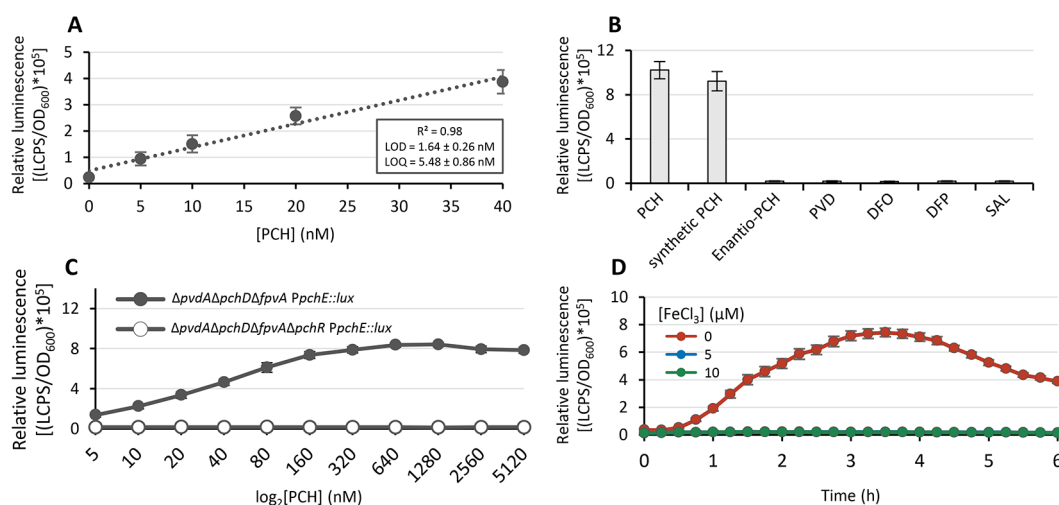


Figure 3. Biosensor response is activated by PchR and is repressed by iron. (A) Linear dose–response plot of the biosensor. Relative light emission values (LCPS/OD₆₀₀) were taken after 3.5 h of incubation at 25 °C in the presence of increasing PCH concentration (0–40 nM). The linear regression line and the R^2 value are shown. The limit of detection (LOD) and limit of quantification (LOQ) were calculated with S/N (signal/noise ratio) values of 3 and 10, respectively. (B) Response of the biosensor to natural PCH from *P. aeruginosa* PAO1, synthetic PCH, enantio-PCH, pyoverdine (PVD), deferoxamine (DFO), deferiprone (DFP), and salicylate (SAL) after 3.5 h of incubation at 25 °C. All chelators were added at the final concentration of 160 nM. (C) Relative light emission (LCPS/OD₆₀₀) by the *P. aeruginosa* $\Delta pvdA\Delta pchD\Delta fvpA$ mutant carrying the *PpchE::lux* fusion (black circle) and by the *P. aeruginosa* $\Delta pvdA\Delta pchD\Delta fvpA\Delta pchR$ mutant carrying the *PpchE::lux* fusion (white circle) in response to increasing PCH concentrations (5 to 5120 nM) after 3.5 h of incubation at 25 °C. (D) Relative light emission (LCPS/OD₆₀₀) by the *P. aeruginosa* $\Delta pvdA\Delta pchD\Delta fvpA$ mutant carrying the *PpchE::lux* fusion in response to 160 nM PCH in the presence of 5 μ M (square), 10 μ M (triangle), or without (circle) FeCl₃. LCPS and OD₆₀₀ were measured every 15 min for 6 h at 25 °C. Data are the mean of three independent experiments \pm SD.

regulator PchR. Under these conditions, the $\Delta pvdA\Delta pchD\Delta fvpA$ *PpchE::lux* biosensor rapidly responded to exogenous PCH, attaining the maximum relative light emission in 3 to 3.5 h after the addition of PCH (Figure 2I). No significant evaporation of the biosensor suspension medium (*i.e.*, volume reduction) was noticed during the experimental time course.

Bioluminescent Cell-Based Biosensor Selectively Responds to PCH, Requires PchR, and Is Repressed by Iron. Since the maximum light emission of the $\Delta pvdA\Delta pchD\Delta fvpA$ *PpchE::lux* biosensor was observed 3.5 h after the addition of PCH, the limit of detection (LOD) and the limit of quantification (LOQ) were determined at this time point. A linear dose–response relationship ($R^2 = 0.98$) in the 5–40 nM range of PCH concentration was observed (Figure 3A). Within this PCH concentration range, the LOD and LOQ values were 1.64 ± 0.26 and 5.48 ± 0.86 nM, respectively (Figure 3A). These analytical performances represent a significant advance over previous PCH quantification methods, which required large sample volumes (mL)^{36,42,55} and eventual concentration after solvent extraction^{36,42} and exhibited sensitivity in the μ M PCH range.¹¹ To investigate the selectivity of the $\Delta pvdA\Delta pchD\Delta fvpA$ *PpchE::lux* biosensor, the luminescence emission was measured upon the addition of several iron-chelating compounds, using the standard test conditions (OD₆₀₀ \approx 0.25; 50 μ L volume; 3.5 h; 25 °C). Purified PCH from *P. aeruginosa* PAO1 and chemically synthesized PCH were included as controls. Each iron-chelating compound (listed in Table S3) was added at 160 nM. As expected, the bioluminescence emission induced by the chemically synthesized PCH was similar to that of the native PCH extracted from *P. aeruginosa* culture supernatants (Figure 3B). Conversely, in the presence of chemically synthesized enantio-PCH, a PCH diastereoisomer was produced by

Pseudomonas protegens,⁵⁶ and the bioluminescence emission was completely abrogated (Figure 3B). The inability of enantio-PCH to induce the expression of PCH genes in *P. aeruginosa* and consequently the biosensor response confirms that enantio-PCH is not recognized by *P. aeruginosa* due to the high specificity of the PCH translocation machinery and of the PchR-mediated gene expression.⁵⁵ No response was also observed with other iron-chelating compounds, namely, PVD, deferoxamine (DFO), deferiprone (DFP), and sodium salicylate (SAL, a PCH precursor), further confirming the biosensor selectivity (Figure 3B). The biosensor genetic circuitry is based on the assumption that the production of PCH is controlled by the cytoplasmic transcriptional regulator PchR, which activates the transcription of PCH biosynthesis and transport genes. To define the role of PchR on the biosensor response, the *pchR* gene was deleted from the $\Delta pvdA\Delta pchD\Delta fvpA$ *PpchE::lux* biosensor strain, and the expression of the *PpchE::lux* fusion was monitored using the standard assay conditions (OD₆₀₀ \approx 0.25; 50 μ L volume; 3.5 h; 25 °C concentration range). As expected, the deletion of *pchR* completely abrogated PCH-inducible *PpchE::lux* expression in the 5–5.120 nM PCH range, confirming that PchR is strictly required in PCH gene expression and thus for the PCH-mediated response of the biosensor (Figure 3C).

To verify the ability of iron to repress the expression of the *PpchE::lux* fusion, the biosensor was exposed to 160 nM of PCH, in the presence of two different FeCl₃ concentrations (*i.e.*, 5 and 10 μ M). The bioluminescence signal emission was completely shut off with 5 μ M FeCl₃ (Figure 3D).

Taken together, these results indicate that the biosensor response depends on the concentration of PCH and iron, in line with the regulatory mechanisms, which control PCH production and uptake.




Figure 4. Factors affecting PCH detection in *P. aeruginosa* culture supernatants. Relative bioluminescence emission of the *P. aeruginosa* $\Delta pvdA\Delta pchD\Delta fpvA PpchE::lux$ biosensor, in the presence of PAO1, $\Delta pvdA$, $\Delta pchD$, and $\Delta pvdA\Delta pchD$ culture supernatants obtained after a 24 h growth in DCAA (A) or in the presence of increasing concentrations of PCH (from 0.625 to 4 μM) and of PVD (from 0.625 to 20 μM) (B). (C) PCH concentrations ($\mu\text{M}/\text{OD}_{600}$) in the diluted (1:1024) supernatants of the indicated *P. aeruginosa* strains grown for 24 h in DCAA. Data are representative of three independent experiments \pm SD.

PVD Interference with PCH Measurement. Several studies in animal models and humans showed that PCH biosynthesis and uptake genes are expressed during *P. aeruginosa* infection,^{25–29} though the presence of PCH could be detected fluorometrically in a few CF sputum samples.^{11,26} Fluorescence spectroscopy can detect PCH concentrations of $>1 \mu\text{M}$, and therefore, with this method, it is not possible to detect PCH in *P. aeruginosa* isolates, which produce lower PCH concentrations (i.e., $<1 \mu\text{M}$).¹¹ Moreover, PCH fluorescence is quenched upon Fe(III) binding,⁵⁷ implying that the Fe(III)-PCH complex escapes fluorometric detection. Another commonly used procedure for PCH quantification entails solvent extraction and purification by HPLC.³⁹ Both these methods are affected by significant analyte loss and unavoidably underestimate the actual concentration of PCH produced by *P. aeruginosa*.

The ability of the biosensor to specifically and rapidly respond to low PCH concentrations encouraged its use for direct PCH quantification in *P. aeruginosa* culture supernatants. Calibration of the biosensor can easily be obtained with commercially available PCH (Santa Cruz Biotechnology Inc., CA). To this purpose, the supernatants of wild-type PAO1 and $\Delta pvdA$ and $\Delta pchD$ single and double mutants were collected after 24 h of growth in the iron-poor medium DCAA, and the biosensor bioluminescence emission was measured. As expected, no bioluminescence emission was recorded in culture supernatants of PCH-defective mutants, indicating that no compound other than PCH can trigger the biosensor (Figure 4A). Surprisingly, the bioluminescence emission of the PAO1 culture supernatant was much lower than that of the $pvdA$ mutant (Figure 4A). This result is in contrast with previous data showing that wild-type PAO1 and PVD defective mutants produce a similar amount of PCH under iron-limited conditions²⁴ and suggests that high PVD levels can interfere with the biosensor response. To verify this hypothesis, PCH was extracted from the supernatant of PAO1, $\Delta pvdA$, $\Delta pchD$, and $\Delta pvdA\Delta pchD$ and analyzed by TLC. The PCH spot of PAO1 was quantitatively similar that of the $pvdA$ mutant (Figure S4A), suggesting that PCH production in these two strains is comparable under the test conditions. Since PAO1 produces a high amount of PVD when grown in DCAA (Figure S4B), we hypothesized that PVD may hamper PCH measurements by chelating iron traces in the growth medium. Indeed, previous work has demonstrated that PchR binds PCH in its iron-loaded form, while it does not in its apo-form.^{21,58} Therefore, iron withholding by PVD could negatively affect

PCH gene expression, and consequently bioluminescence emission. To verify this hypothesis, the biosensor response was measured in the presence of increasing concentrations of purified PCH and PVD (62.5–4000 and 20–20,000 nM, respectively). The choice of using 20,000 nM as the maximum PVD concentration derives from the experimental observation that *P. aeruginosa* PAO1 produces $\approx 200 \mu\text{M}$ PVD in DCAA culture supernatants (Figure S4B) and that a 1:10 dilution (i.e., 5 μL of culture supernatants added to 45 μL of biosensor suspension) is used for the assay. PVD concentrations of ≥ 2500 nM significantly reduced the biosensor luminescence emission (Figure 4B), even in the presence of elevated PCH concentrations. Conversely, PVD concentrations of ≤ 1250 nM had a negligible effect on the biosensor luminescence emission at all PCH concentrations tested. The above findings suggest that an appropriate dilution of *P. aeruginosa* culture supernatants can overcome PVD interference in the PCH biosensor assay. To corroborate these results, the culture supernatants of wild-type PAO1 and $\Delta pvdA$ and $\Delta pchD$ single and double mutants were serially diluted, and the bioluminescence emission of the $\Delta pvdA\Delta pchD\Delta fpvA PpchE::lux$ biosensor was measured after 3.5 h at 25 °C. Interestingly, the luminescence emission progressively increased with serial dilution of the PAO1 supernatant, reaching the same values of the PVD-deficient $\Delta pvdA$ mutant at 1:32 dilution (Figure S5A). Moreover, the biosensor luminescence emission in the presence of the $\Delta pvdA$ mutant supernatant was nearly constant up to the 1:32 dilution, suggesting that PCH levels in supernatants of the PVD-defective mutant exceeded the upper detection limit of the biosensor, resulting in its saturation.

The above results indicate that an appropriate dilution of culture supernatants is mandatory for PCH quantification. To calculate the concentration of PCH produced by *P. aeruginosa*, 1:256, 1:512, and 1:1024 dilutions were used, and the PCH concentration was calculated by using a standard calibration curve (Figure S5B). Interestingly, the PCH concentrations estimated by using the three different dilutions gave comparable results (Figure S5C), as expected for PCH concentrations below the biosensor saturation point (i.e., 160 nM, Figure 2I and Figure 3C). Therefore, the lowest sample dilution (1:1024) was selected for further experiments (see also the Supporting Information, text S1). By diluting the supernatant, the PCH concentrations determined for PAO1 and the $\Delta pvdA$ mutant culture supernatants ($\approx 70 \mu\text{M}/\text{OD}_{600}$) were in line with previous experiments (Figure 4C) and literature data.⁵⁹




Figure 5. Bioassays for PCH detection in liquid and solid media. (A) PCH concentrations ($\mu\text{M}/\text{OD}_{600}$) in the culture supernatants of *P. aeruginosa* strains PAO1, ATCC 27853, LesB58, and TR1 grown in DCAA for 24 h. Supernatants were 1:1024 diluted, and PCH concentration was calculated using a PCH calibration curve, as outlined in the Supporting Information, text S1. Data are representative of three independent experiments \pm SD. (B) Top: qualitative detection of PCH production on CAA agarose plates, as outlined in the Supporting Information, text S2. *P. aeruginosa* strains were spotted on CAA agarose plates, grown for 24 h at 37 °C, and killed by chloroform vapor. Then, CAA agarose plates were overlaid with the *P. aeruginosa* $\Delta\text{pvdA}\Delta\text{pchD}\Delta\text{fpvA}$ *PpchE::lux* biosensor strain and incubated for 1 h at 37 °C. The PCH grey halo was detected using a ChemiDoc XRS+ Imaging System (Bio-Rad). The gray scale denotes pixel intensity. Bottom: PVD production by the *P. aeruginosa* strain, prior to the biosensor overlay, detected as fluorescence emission upon UV light exposure. Images are representative of one of several independent tests providing similar results.




Figure 6. Biosensor response to PCH-spiked biological fluids. Relative light emission (LCPS/OD₆₀₀) of the *P. aeruginosa* $\Delta\text{pvdA}\Delta\text{pchD}\Delta\text{fpvA}$ *PpchE::lux* biosensor in response to increasing concentrations of PCH (5 to 5120 nM) in undiluted and diluted (10^{-1} and 10^{-2}) biological fluids, after 3.5 h of incubation at 25 °C. Each value represents the mean \pm SD of three independent experiments.

PCH Quantification in *P. aeruginosa* Clinical Strains and Biological Fluids. To check the ability of the biosensor to measure PCH levels produced by clinical *P. aeruginosa* strains, *P. aeruginosa* ATCC 27853⁶⁰ and the Liverpool-epidemic strain LesB58⁶¹ were preliminarily tested. *P. aeruginosa* ATCC 27853 and LesB58 produce different PVD types (i.e., type II and III PVD, respectively) and release quite different PVD levels in the medium (Figure S4B). *P. aeruginosa* strains were cultured for 24 h in DCAA, and the supernatants were diluted. The biosensor response to the supernatant of ATCC 27853 was similar to that observed with PAO1, showing biosensor saturation and PVD interference for $\leq 1:32$ supernatant dilution. Contrarily, the supernatant of LesB58 determined an initial increase (2-fold dilution) of bioluminescence emission, which remained constant up to the 64-fold dilution (Figure S5D). The different response profile can be ascribed to the different PVD concentrations in the supernatants of two test strains (Figure S4B). Indeed, the amount of PVD produced by PAO1 and ATCC 27853 under iron-poor conditions is almost the same ($\sim 200 \mu\text{M}$), while the PVD concentration in the LesB58 supernatant is 10-fold lower (Figure S4B). These findings further corroborate the need of eliminating PVD interference by diluting the supernatant prior to PCH measurement. On this basis, to calculate the exact concentration of PCH produced by PAO1, ATCC 27853, and LesB58, culture supernatants were diluted 1:1024, and 5 μL of each supernatant were used for the assay, as recommended in

the Supporting Information, text S1. Preliminary dilution lowers the PVD concentration to $<40 \text{ nM}$, thereby preventing any interference of PVD with biosensor response to PCH (Figure 4B). The clinical *P. aeruginosa* isolate TR1 was included as a negative control, being a natural PCH-defective mutant.⁶² Interestingly, PCH production was slightly lower in *P. aeruginosa* LesB58 than in ATCC 27853 and PAO1, while no PCH was detected in the supernatant of the PCH-negative strain TR1 (Figure 5A). Altogether, these results indicate that, with an appropriate setting (Supporting Information, text S1), the biosensor is a valuable tool to quantify PCH production by *P. aeruginosa* clinical isolates.

Lastly, the newly generated whole-cell biosensor was adapted to generate a rapid screening system of PCH-producing *P. aeruginosa* strains on solid media. To this aim, several *P. aeruginosa* strains (listed in Table S1) were spot-inoculated on CAA agarose plates and grown at 37 °C for 24 h until $\sim 3 \text{ mm}$ colonies became visible. Colonies were inspected under UV light exposure to detect PVD production (blue halo), and then bacteria were killed with chloroform vapors. Thereafter, a thin ($\sim 1 \text{ mm}$) agarose layer containing the $\Delta\text{pvdA}\Delta\text{pchD}\Delta\text{fpvA}$ *PpchE::lux* biosensor was overlaid onto the test colonies and bioluminescence emission was detected after 1 h incubation at 37 °C. To validate the plate-based screening system, wild-type *P. aeruginosa* PAO1 and PCH and/or PVD defective mutants were tested. Noteworthy, the same signal was registered for wild-type *P. aeruginosa* PAO1 and

PVD-null mutant $\Delta pvdA$, (Figure 5B), while no light emission was observed for $\Delta pchD$, $\Delta pvdA\Delta pchD$, and TR1 PCH-null mutants (Figure 5B). Although with some differences, probably due to growth rate variations and PVD production levels (Figure 5B, bottom), all clinical strains tested positive for PCH production (Figure 5B).

The PCH plate assay was then applied to the screening of 98 *P. aeruginosa* clinical isolates from CF patients at different stages of lung infection. The vast majority of isolates produced both siderophores (Table S4); PVD- and PCH-negative isolates were only 16.3 and 7.1%, respectively, with two isolates testing double-negative.

The biosensor performances were also tested using sputum, artificial tears, and urine as input samples, upon spiking with known PCH concentrations (5 to 5120 nM). While undiluted fluids significantly reduced the biosensor response, negligible interference was observed for 10- and 100-fold diluted fluids (Figure 6).

Interestingly, transcription of *pch* biosynthetic genes was previously demonstrated in the majority of CF sputa, though PCH was detected in only 13% of them, likely due to the poor sensitivity of the PCH detection method ($\sim 1 \mu\text{M}$).²⁶ Here, pilot testing of sputa from eight anonymous CF patients revealed that PCH was detectable in six of them (range 86.9 ± 4.6 – $24,390.0 \pm 91.2$ nM), showing an excellent correlation between the presence of PCH and *P. aeruginosa* culture-positivity of sputa (Table S5).

Altogether, these results indicate that the $\Delta pvdA\Delta pchD\Delta fpvA$ *PpchE::lux* biosensor is suitable for PCH quantification in both *P. aeruginosa* culture supernatants and biological fluids and can be used for the rapid screening of PCH-producing *P. aeruginosa* isolates on a solid medium (Supporting Information, text S2).

CONCLUSIONS

In summary, we generated a whole cell-based biosensor for PCH quantification and tested its proficiency under laboratory conditions. The biosensor specificity is guaranteed by the unique selectivity of the PCH transport machinery and the PchR activator of the *PpchE::lux* reporter fusion. In fact, both the FptA receptor and the PchR regulator are strictly PCH-selective.^{58,63} Accordingly, evidence was provided that the biosensor does not respond to PCH stereoisomers or precursors, as well as to a variety of iron-chelating compounds, excluding the possibility of false positive readouts.

Two main factors, namely, iron and PVD carryover in the test sample, were shown to interfere with the biosensor performances. Both factors, however, do not undermine the biosensor validity by virtue of the extremely high sensitivity of the assay (lower detection limit = 1.64 ± 0.26 nM PCH), which requires the sample to be diluted several fold ($\cong 10^{-3}$) prior to testing, so that interference by iron and PVD would be negligible. It should also be taken into account that PCH is produced by *P. aeruginosa* only under conditions of severe iron limitation [$< 5 \mu\text{M Fe(III)}$],⁴⁰ implying that the presence of sufficient ($\geq 5 \mu\text{M}$) iron levels in biological samples would be incompatible with PCH production by *P. aeruginosa*. In practice, considering that the concentration of secreted PCH is extremely variable depending on the *P. aeruginosa* strain and growth conditions (from $\sim 800,000$ to ~ 1000 nM in optimized laboratory media and CF sputa, respectively),^{11,34} appropriate serial dilutions of the sample should be made to adjust the PCH concentration in the linear response range of the

biosensor (5–40 nM; Figure 3A). Of note, a calibration curve can be easily prepared using pure PCH, which is commercially available.

The luminescent biosensor offers several advantages over previous PCH detection and/or quantification methods, which rely on chromatographic or spectrophotometric analysis of partially purified organic extracts. Briefly, (i) the assay protocol is straightforward and allows PCH to be quantified in 3.5 h with negligible sample handling; (ii) up to 28 samples can contemporarily be tested in triplicate using a single 96-well microplate, also including standard samples for system calibration; (iii) the microtiter plate format would allow the assay to be scaled down to a smaller format for higher throughput (e.g., using 384-well microplates) and is amenable to automation (e.g., using automatic dispensers); (iv) once dispensed with the reporter strain, the microtiter plates can be stored frozen at -80°C for months with negligible loss of the assay performances (Figure S6); (v) the assay combines high sensitivity (LOQ in the nM PCH range) with simplicity, since the luciferase-based reporter system is characterized by a high signal/noise ratio and does not require an exogenous substrate for signal emission. Bioluminescence background levels in living cells are extremely low, making bioluminescence up to 50 times more sensitive than fluorescence, which would be impracticable in testing the intrinsically fluorescent *Pseudomonas* species.^{52,64} Moreover, *P. luminescens* luciferase is endowed with remarkable chemical and physical stability.⁶⁵

The inclusion of *P. aeruginosa* into the list of risk group 2 bacterial pathogens could represent a limitation to the use of the luminescent biosensor in biosafety level 1 laboratories. However, the *P. aeruginosa* PAO1 $\Delta pvdA\Delta pchD\Delta fpvA$ mutant carries stable genetic knock-outs of both PCH and PVD biosynthesis genes, together with a deletion of the PVD receptor gene. Altogether, these mutations impair iron uptake and result in an avirulent phenotype in animal models of infections,^{24,66,67} downgrading the risk associated with biosensor manipulation.

In conclusion, the $\Delta pvdA\Delta pchD\Delta fpvA$ *PpchE::lux* whole cell-based biosensor represents an innovative tool to detect and quantify the PCH siderophore. The preliminary setup of the test conditions allows the fast, easy, accurate, and cost-effective determination of nanomolar PCH concentrations in *P. aeruginosa* liquid cultures and biological fluids, as well as the qualitative screening of PCH-producing *P. aeruginosa* colonies on an agar plate, hopefully facilitating future investigations on the role of PCH in the pathogenesis of *P. aeruginosa* infection.

ASSOCIATED CONTENT

Supporting Information

The Supporting Information is available free of charge at <https://pubs.acs.org/doi/10.1021/acssensors.1c01023>.

Supplementary methods, figures, tables, and description of the analytical protocol (PDF)

AUTHOR INFORMATION

Corresponding Authors

Daniela Visaggio – Department of Science, Roma Tre University, Rome 00146, Italy; Santa Lucia Foundation IRCCS, Rome 00179, Italy; Email: daniela.visaggio@uniroma3.it

Paolo Visca – Department of Science, Roma Tre University, Rome 00146, Italy; Santa Lucia Foundation IRCCS, Rome

00179, Italy; orcid.org/0000-0002-6128-7039;
Email: paolo.visca@uniroma3.it

Authors

Mattia Pirollo – Department of Science, Roma Tre University, Rome 00146, Italy; Present Address: Department of Veterinary and Animal Sciences, University of Copenhagen, DK-1165 Frederiksberg, Denmark

Emanuela Frangipani – Department of Biomolecular Sciences, University of Urbino Carlo Bo, Urbino 61029, Italy; orcid.org/0000-0001-5619-7912

Massimiliano Lucidi – Department of Science, Roma Tre University, Rome 00146, Italy

Raffaella Sorrentino – Department of Molecular Medicine and Medical Biotechnology, University of Naples Federico II, Naples 80138, Italy

Emma Mitidieri – Department of Molecular Medicine and Medical Biotechnology, University of Naples Federico II, Naples 80138, Italy

Francesca Ungaro – Department of Pharmacy, University of Naples Federico II, Naples 80131, Italy; orcid.org/0000-0003-0850-9533

Andrea Luraghi – Department of Biotechnology and Biosciences, University of Milano-Bicocca, Milan 20126, Italy

Francesco Peri – Department of Biotechnology and Biosciences, University of Milano-Bicocca, Milan 20126, Italy; orcid.org/0000-0002-3417-8224

Complete contact information is available at:

<https://pubs.acs.org/10.1021/acssensors.1c01023>

Author Contributions

E.F. and P.V. conceived and designed the study. D.V., M.P., M.L., A.L., and E.M. performed the experiments. E.F., R.S., F.U., F.P., and P.V. analyzed the results. D.V., E.F., F.P., and P.V. wrote the manuscript. All authors have given approval to the final version of the manuscript.

Author Contributions

[‡]D.V. and M.P. contributed equally to this work.

Funding

This work was supported by grants FFC#21/2015 and FFC#18/2017 from the Italian Cystic Fibrosis Research Foundation, and grant PRIN 2017 Prot. 20177J5Y3P from the Italian Ministry of Education, University and Research (MIUR), to P.V.

Notes

The authors declare no competing financial interest.

ABBREVIATIONS

CAA, casamino acids; DCAA, deferrated casamino acids; DFP, deferiprone; DFO, deferoxamine; DMSO, dimethyl sulfoxide; Fur, ferric uptake regulator protein; HPLC, high-performance liquid chromatography; LB, Luria-Bertani broth; LCPS, light counts per second; LOD, limit of detection; LOQ, limit of quantification; PVD, pyoverdine; PCH, pyochelin; S, slope of calibration curve; SAL, salicylate; S/N, signal/noise ratio; SD, standard deviation; TLC, thin layer chromatography

REFERENCES

- (1) Ganz, T. Iron in Innate Immunity: Starve the Invaders. *Curr. Opin. Immunol.* **2009**, *21*, 63–67.
- (2) Carver, P. L. The Battle for Iron between Humans and Microbes. *Curr. Med. Chem.* **2018**, *25*, 85–96.

- (3) Krewulak, K. D.; Vogel, H. J. Structural Biology of Bacterial Iron Uptake. *Biochim. Biophys. Acta, Biomembr.* **2008**, *1778*, 1781–1804.

- (4) Lamont, I. L.; Konings, A. F.; Reid, D. W. Iron Acquisition by *Pseudomonas aeruginosa* in the Lungs of Patients with Cystic Fibrosis. *BioMetals* **2009**, *22*, 53–60.

- (5) Lyczak, J. B.; Cannon, C. L.; Pier, G. B. Lung Infections Associated with Cystic Fibrosis. *Clin. Microbiol. Rev.* **2002**, *15*, 194–222.

- (6) Cox, C. D.; Adams, P. Siderophore Activity of Pyoverdine for *Pseudomonas aeruginosa*. *Infect. Immun.* **1985**, *48*, 130–138.

- (7) Liu, P. V.; Shokrani, F. Biological Activities of Pyochelins: Iron-Chelating Agents of *Pseudomonas aeruginosa*. *Infect. Immun.* **1978**, *22*, 878–890.

- (8) Albrecht-Gary, A. M.; Blanc, S.; Rochel, N.; Ocaktan, A. Z.; Abdallah, M. A. Bacterial Iron Transport: Coordination Properties of Pyoverdine PaA, a Peptidic Siderophore of *Pseudomonas aeruginosa*. *Inorg. Chem.* **1994**, *33*, 6391–6402.

- (9) Visca, P.; Imperi, F.; Lamont, I. L. Pyoverdine Siderophores: From Biogenesis to Biosignificance. *Trends Microbiol.* **2007**, *15*, 22–30.

- (10) Haas, B.; Kraut, J.; Marks, J.; Zanker, S. C.; Castignetti, D. Siderophore Presence in Sputa of Cystic Fibrosis Patients. *Infect. Immun.* **1991**, *59*, 3997–4000.

- (11) Martin, L. W.; Reid, D. W.; Sharples, K. J.; Lamont, I. L. *Pseudomonas* Siderophores in the Sputum of Patients with Cystic Fibrosis. *BioMetals* **2011**, *24*, 1059–1067.

- (12) Ankenbauer, R. G.; Cox, C. D. Isolation and Characterization of *Pseudomonas aeruginosa* Mutants Requiring Salicylic Acid for Pyochelin Biosynthesis. *J. Bacteriol.* **1988**, *170*, 5364–5367.

- (13) Serino, L.; Reimann, C.; Baur, H.; Beyeler, M.; Visca, P.; Haas, D. Structural Genes for Salicylate Biosynthesis from Chorismate in *Pseudomonas aeruginosa*. *Mol. Gen. Genet.* **1995**, *249*, 217–228.

- (14) Serino, L.; Reimann, C.; Visca, P.; Beyeler, M.; Chiesa, V. D.; Haas, D. Biosynthesis of Pyochelin and Dihydroaeruginic Acid Requires the Iron-Regulated *pchDCBA* Operon in *Pseudomonas aeruginosa*. *J. Bacteriol.* **1997**, *179*, 248–257.

- (15) Schlegel, K.; Taraz, K.; Budzikiewicz, H. The Stereoisomers of Pyochelin, a Siderophore of *Pseudomonas aeruginosa*. *BioMetals* **2004**, *17*, 409–414.

- (16) Brandel, J.; Humbert, N.; Elhabiri, M.; Schalk, I. J.; Mislin, G. L.; Albrecht-Gary, A. M. Pyochelin, a Siderophore of *Pseudomonas aeruginosa*: Physicochemical Characterization of the Iron(III), Copper(II) and Zinc(II) complexes. *Dalton Trans.* **2012**, *41*, 2820–2834.

- (17) Ronnebaum, T. A.; Lamb, A. L. Nonribosomal Peptides for Iron Acquisition: Pyochelin Biosynthesis as a Case Study. *Curr. Opin. Struct. Biol.* **2018**, *53*, 1–11.

- (18) Cunrath, O.; Gasser, V.; Hoegy, F.; Reimann, C.; Guillon, L.; Schalk, I. J. A Cell Biological View of the Siderophore Pyochelin Iron Uptake Pathway in *Pseudomonas aeruginosa*. *Environ. Microbiol.* **2015**, *17*, 171–185.

- (19) Reimann, C. Inner-Membrane Transporters for the Siderophores Pyochelin in *Pseudomonas aeruginosa* and Enantio-Pyochelin in *Pseudomonas fluorescens* Display Different Enantioselectivities. *Microbiology* **2012**, *158*, 1317–1324.

- (20) Heinrichs, D. E.; Poole, K. PchR, a Regulator of Ferripyochelin Receptor Gene (FptA) Expression in *Pseudomonas aeruginosa*, Functions Both as an Activator and as a Repressor. *J. Bacteriol.* **1996**, *178*, 2586–2592.

- (21) Michel, L.; González, N.; Jagdeep, S.; Nguyen-Ngoc, T.; Reimann, C. PchR-Box Recognition by the AraC-Type Regulator PchR of *Pseudomonas aeruginosa* Requires the Siderophore Pyochelin as an Effector. *Mol. Microbiol.* **2005**, *58*, 495–509.

- (22) Reimann, C.; Serino, L.; Beyeler, M.; Haas, D. Dihydroaeruginic Acid Synthetase and Pyochelin Synthetase, Products of the *pchEF*, Are Induced by Extracellular Pyochelin in *Pseudomonas aeruginosa*. *Microbiology* **1998**, *144*, 3135–3148.

- (23) Palmer, L. D.; Skaar, E. P. Transition Metals and Virulence in Bacteria. *Annu. Rev. Genet.* **2016**, *50*, 67–91.

- (24) Minandri, F.; Imperi, F.; Frangipani, E.; Bonchi, C.; Visaggio, D.; Facchini, M.; Pasquali, P.; Bragonzi, A.; Visca, P. Role of Iron Uptake Systems in *Pseudomonas aeruginosa* Virulence and Airway Infection. *Infect. Immun.* **2016**, *84*, 2324–2335.
- (25) Kim, M.; Christley, S.; Khodarev, N. N.; Fleming, I.; Huang, Y.; Chang, E.; Zaborina, O.; Alverdy, J. *Pseudomonas aeruginosa* Wound Infection Involves Activation of Its Iron Acquisition System in Response to Fascial Contact. *J. Trauma Acute Care Surg.* **2015**, *78*, 823–829.
- (26) Konings, A. F.; Martin, L. W.; Sharples, K. J.; Roddam, L. F.; Latham, R.; Reid, D. W.; Lamont, I. L. *Pseudomonas aeruginosa* Uses Multiple Pathways To Acquire Iron during Chronic Infection in Cystic Fibrosis Lungs. *Infect. Immun.* **2013**, *81*, 2697–2704.
- (27) Kruczek, C.; Kottapalli, K. R.; Dissanaik, S.; Dzvova, N.; Griswold, J. A.; Colmer-Hamood, J. A.; Hamood, A. N. Major Transcriptome Changes Accompany the Growth of *Pseudomonas aeruginosa* in Blood from Patients with Severe Thermal Injuries. *PLoS One* **2016**, *11*, No. e0149229.
- (28) Tielen, P.; Rosin, N.; Meyer, A.-K.; Dohnt, K.; Haddad, I.; Jänsch, L.; Klein, J.; Narten, M.; Pommerenke, C.; Scheer, M.; Schobert, M.; Schomburg, D.; Thielen, B.; Jahn, D. Regulatory and Metabolic Networks for the Adaptation of *Pseudomonas aeruginosa* Biofilms to Urinary Tract-Like Conditions. *PLoS One* **2013**, *8*, No. e71845.
- (29) Wang, J.; Mushegian, A.; Lory, S.; Jin, S. Large-Scale Isolation of Candidate Virulence Genes of *Pseudomonas aeruginosa* by in Vivo Selection. *Proc. Natl. Acad. Sci. U. S. A.* **1996**, *93*, 10434–10439.
- (30) Britigan, B. E.; Roeder, T. L.; Rasmussen, G. T.; Shasby, D. M.; McCormick, M. L.; Cox, C. D. Interaction of the *Pseudomonas aeruginosa* Secretory Products Pyocyanin and Pyochelin Generates Hydroxyl Radical and Causes Synergistic Damage to Endothelial Cells. Implications for *Pseudomonas*-Associated Tissue Injury. *J. Clin. Invest.* **1992**, *90*, 2187–2196.
- (31) Coffman, T. J.; Cox, C. D.; Edeker, B. L.; Britigan, B. E. Possible Role of Bacterial Siderophores in Inflammation. Iron Bound to the *Pseudomonas* Siderophore Pyochelin Can Function as a Hydroxyl Radical Catalyst. *J. Clin. Invest.* **1990**, *86*, 1030–1037.
- (32) Cox, C. D. Iron Uptake with Ferripyochelin and Ferric Citrate by *Pseudomonas aeruginosa*. *J. Bacteriol.* **1980**, *142*, 581–587.
- (33) Hoegy, F.; Mislin, G. L. A.; Schalk, I. J. Pyoverdine and Pyochelin Measurements. *Methods Mol. Biol.* **2014**, *1149*, 293–301.
- (34) Reimmann, C.; Patel, H. M.; Serino, L.; Barone, M.; Walsh, C. T.; Haas, D. Essential PchG-Dependent Reduction in Pyochelin Biosynthesis of *Pseudomonas aeruginosa*. *J. Bacteriol.* **2001**, *183*, 813–820.
- (35) Sambrook, J.; Fritsch, E. F.; Maniatis, T. *Molecular Cloning: A Laboratory Manual*; Cold Spring Harbor Laboratory Press, 1989, No. Ed. 2.
- (36) Visca, P.; Ciervo, A.; Sanfilippo, V.; Orsi, N. Iron-Regulated Salicylate Synthesis by *Pseudomonas* Spp. *Microbiology* **1993**, *139*, 1995–2001.
- (37) Visca, P.; Serino, L.; Orsi, N. Isolation and Characterization of *Pseudomonas aeruginosa* Mutants Blocked in the Synthesis of Pyoverdine. *J. Bacteriol.* **1992**, *174*, 5727–5731.
- (38) Bonchi, C.; Frangipani, E.; Imperi, F.; Visca, P. Pyoverdine and Proteases Affect the Response of *Pseudomonas aeruginosa* to Gallium in Human Serum. *Antimicrob. Agents Chemother.* **2015**, *59*, 5641–5646.
- (39) Porcaro, F.; Bonchi, C.; Ugolini, A.; Frangipani, E.; Polzonetti, G.; Visca, P.; Meneghini, C.; Battocchio, C. Understanding the Biomimetic Properties of Gallium in *Pseudomonas aeruginosa*: An XAS and XPS Study. *Dalton Trans.* **2017**, *46*, 7082–7091.
- (40) Visca, P.; Colotti, G.; Serino, L.; Verzili, D.; Orsi, N.; Chiancone, E. Metal Regulation of Siderophore Synthesis in *Pseudomonas aeruginosa* and Functional Effects of Siderophore-Metal Complexes. *Appl. Environ. Microbiol.* **1992**, *58*, 2886–2893.
- (41) Zhang, S.; Chen, Y.; Potvin, E.; Sanschagrin, F.; Levesque, R. C.; McCormack, F. X.; Lau, G. W. Comparative Signature-Tagged Mutagenesis Identifies *Pseudomonas* Factors Conferring Resistance to the Pulmonary Collectin SP-A. *PLoS Pathog.* **2005**, *1*, No. e31.
- (42) Cox, C. D.; Graham, R. Isolation of an Iron-Binding Compound from *Pseudomonas aeruginosa*. *J. Bacteriol.* **1979**, *137*, 357–364.
- (43) Patel, H. M.; Tao, J.; Walsh, C. T. Epimerization of an L-Cysteinylyl to a d-Cysteinylyl Residue during Thiazoline Ring Formation in Siderophore Chain Elongation by Pyochelin Synthetase from *Pseudomonas aeruginosa*. *Biochemistry* **2003**, *42*, 10514–10527.
- (44) Venkateswara Rao, B.; Dhokale, S.; Rajamohanam, P. R.; Hotha, S. A Tetrazine Templated Method for the Synthesis of Ternary Conjugates. *Chem. Commun.* **2013**, *49*, 10808–10810.
- (45) Zamri, A.; Abdallah, M. A. An Improved Stereocontrolled Synthesis of Pyochelin, Siderophore of *Pseudomonas aeruginosa* and *Burkholderia cepacia*. *Tetrahedron* **2000**, *56*, 249–256.
- (46) Milton, D. L.; O'Toole, R.; Horstedt, P.; Wolf-Watz, H. Flagellin A Is Essential for the Virulence of *Vibrio anguillarum*. *J. Bacteriol.* **1996**, *178*, 1310–1319.
- (47) Voisard, C.; Bull, C.; Keel, C.; Laville, J.; Maurhofer, M.; Schnider, U.; Défago, G.; Haas, D.; In O'Gara, F.; Dowling, D. N.; Boesten, B. (Eds) *Molecular Ecology of Rhizosphere Microorganisms*; AGRIS, 1994, 67–89.
- (48) Hoang, T. T.; Kutchma, A. J.; Becher, A.; Schweizer, H. P. Integration-Proficient Plasmids for *Pseudomonas aeruginosa*: Site-Specific Integration and Use for Engineering of Reporter and Expression Strains. *Plasmid* **2000**, *43*, 59–72.
- (49) Liang, G.; Zhao, Z.; Wei, Y.; Liu, K.; Hou, W.; Duan, Y. Plasma Enhanced Label-Free Immunoassay for Alpha-Fetoprotein Based on a U-Bend Fiber-Optic LSPR Biosensor. *RSC Adv.* **2015**, *5*, 23990–23998.
- (50) Webster, T. A.; Sismaet, H. J.; Conte, J. L.; Chan, I. J.; Goluch, E. D. Electrochemical Detection of *Pseudomonas aeruginosa* in Human Fluid Samples via Pyocyanin. *Biosens. Bioelectron.* **2014**, *60*, 265–270.
- (51) Craney, A.; Hohenauer, T.; Xu, Y.; Navani, N. K.; Li, Y.; Nodwell, J. A Synthetic *luxCDABE* Gene Cluster Optimized for Expression in High-GC Bacteria. *Nucleic Acids Res.* **2007**, *35*, No. e46.
- (52) Welsh, D. K.; Noguchi, T. Cellular Bioluminescence Imaging. *Cold Spring Harbor Protoc.* **2012**, *2012*, pdb.top070607.
- (53) Becher, A.; Schweizer, H. P. Integration-Proficient *Pseudomonas aeruginosa* Vectors for Isolation of Single-Copy Chromosomal LacZ and Lux Gene Fusions. *BioTechniques* **2000**, *29*, 948–952.
- (54) Stevenson, K.; McVey, A. F.; Clark, I. B. N.; Swain, P. S.; Pilizota, T. General Calibration of Microbial Growth in Microplate Readers. *Sci. Rep.* **2016**, *6*, 38828.
- (55) Cunrath, O.; Graulier, G.; Carballido-Lopez, A.; Pérard, J.; Forster, A.; Geoffroy, V. A.; Saint, A. P.; Bumann, D.; Mislin, G. L. A.; Michaud-Soret, I.; Schalk, I. J.; Fechter, P. The Pathogen *Pseudomonas aeruginosa* Optimizes the Production of the Siderophore Pyochelin Upon Environmental Challenges. *Metallomics* **2020**, *12*, 2108–2120.
- (56) Youard, Z. A.; Mislin, G. L. A.; Majcherzyk, P. A.; Schalk, I. J.; Reimmann, C. *Pseudomonas* Fluorescens CHA0 Produces Enantio-Pyochelin, the Optical Antipode of the *Pseudomonas aeruginosa* Siderophore Pyochelin. *J. Biol. Chem.* **2007**, *282*, 35546–35553.
- (57) Braud, A.; Hannauer, M.; Mislin, G. L. A.; Schalk, I. J. The *Pseudomonas aeruginosa* Pyochelin-Iron Uptake Pathway and Its Metal Specificity. *J. Bacteriol.* **2009**, *191*, 3517–3525.
- (58) Lin, P.-C.; Youard, Z. A.; Reimmann, C. In Vitro-Binding of the Natural Siderophore Enantiomers Pyochelin and Enantiopyochelin to Their AraC-Type Regulators PchR in *Pseudomonas*. *BioMetals* **2013**, *26*, 1067–1073.
- (59) Cunrath, O.; Geoffroy, V. A.; Schalk, I. J. Metallome of *Pseudomonas aeruginosa*: A Role for Siderophores. *Environ. Microbiol.* **2016**, *18*, 3258–3267.
- (60) Medeiros, A. A.; O'Brien, T. F.; Wacker, W. E. C.; Yulug, N. F. Effect of Salt Concentration on the Apparent In-Vitro Susceptibility of *Pseudomonas* and Other Gram-Negative Bacilli to Gentamicin. *J. Infect. Dis.* **1971**, *124*, S59–S64.
- (61) Cheng, K.; Smyth, R. L.; Govan, J. R.; Doherty, C.; Winstanley, C.; Denning, N.; Heaf, D. P.; van Saene, H.; Hart, C. A. Spread of β-

Lactam-Resistant *Pseudomonas aeruginosa* in a Cystic Fibrosis Clinic. *Lancet*. **1996**, *348*, 639–642.

(62) Frangipani, E.; Bonchi, C.; Minandri, F.; Imperi, F.; Visca, P. Pyochelin Potentiates the Inhibitory Activity of Gallium on *Pseudomonas aeruginosa*. *Antimicrob. Agents Chemother.* **2014**, *58*, 5572–5575.

(63) Hoegy, F.; Lee, X.; Noel, S.; Rognan, D.; Mislin, G. L. A.; Reimann, C.; Schalk, I. J. Stereospecificity of the Siderophore Pyochelin Outer Membrane Transporters in Fluorescent *Pseudomonads*. *J. Biol. Chem.* **2009**, *284*, 14949–14957.

(64) Fila, G.; Krychowiak, M.; Rychlowski, M.; Bielawski, K. P.; Grinholc, M. Antimicrobial Blue Light Photoinactivation of *Pseudomonas aeruginosa*: Quorum Sensing Signaling Molecules, Biofilm Formation and Pathogenicity. *J. Biophotonics* **2018**, *11*, No. e201800079.

(65) Szittner, R.; Meighen, E. Nucleotide Sequence, Expression, and Properties of Luciferase Coded by *lux* Genes from a Terrestrial Bacterium. *J. Biol. Chem.* **1990**, *265*, 16581–16587.

(66) Meyer, J. M.; Neely, A.; Stintzi, A.; Georges, C.; Holder, I. A. Pyoverdinin Is Essential for Virulence of *Pseudomonas aeruginosa*. *Infect. Immun.* **1996**, *64*, 518–523.

(67) Takase, H.; Nitani, H.; Hoshino, K.; Otani, T. Impact of Siderophore Production on *Pseudomonas aeruginosa* Infections in Immunosuppressed Mice. *Infect. Immun.* **2000**, *68*, 1834–1839.